

# Optoelectronic Trapping of Cells, Nanowires, and Nanoparticles

Ming C. Wu

Electrical Engineering and Computer Sciences Department and Berkeley Sensor and Actuator Center (BSAC)

University of California, Berkeley, CA 94720, U.S.A.

Email: wu@eecs.berkeley.edu

**Abstract:** The principle and recent experimental results of optoelectronic tweezers (OET) will be presented. Based on light-induced dielectrophoresis, OET can trap and sort colloidal particles, biological cells, nanowires and nanoparticles using a digital light projector.

©2009 Optical Society of America

**OCIS codes:** (170.4520) Optical confinement and manipulation; (350.4855) Optical tweezers or optical manipulation

## 1. Introduction

The ability to manipulate biological cells, micro- and nanoscopic particles plays an important role in many biological and colloidal science applications. However, conventional manipulation techniques - including optical tweezers, electrophoresis, dielectrophoresis (DEP), magnetic tweezers, acoustic traps, and hydrodynamic flows - cannot achieve high resolution and high throughput at the same time. We have proposed a new technique called optoelectronic tweezers (OET) that permits parallel addressing of individual particles over a large area (Fig. 1) [1]. Using optically induced DEP, OET combines the aspects of both optical tweezers and DEP. The optical power density requirement ( $\sim 0.1$  to  $10 \text{ W/cm}^2$ ) is significantly lower than that of optical tweezers (by four to five orders of magnitude), thanks to the optoelectronic gain in OET. These optical intensities can be achieved by a computer projector, allowing the creation of complex optical manipulation patterns. OET manipulation has been demonstrated on a variety of microparticles including polystyrene beads [1-3], *E. coli* bacteria [4], red and white blood cells [3], HeLa cells [2, 5], and yeast cells [6]. Particle and cell sorting [2, 7] and concentration [8, 9] have also been demonstrated. By controlling bias voltage, we have also shown it is possible to perform light-induced electroporation [10]. A detailed description of the OET devices can be found in [2, 3]. Cell manipulation in highly conductive physiological buffer solution is achieved by replacing amorphous Si photoconductor with phototransistor, which has 100x higher photoconductivity [11]. Recently, OET has been extended to manipulate nanoscopic particles, including semiconducting and metallic nanowires [12] and gold nanoparticles with size as small as 60 nm [13]. Combining OET with surface immobilization techniques, a novel technique called NanoPen has been reported for flexible light "printing" of gold nanoparticles [14].

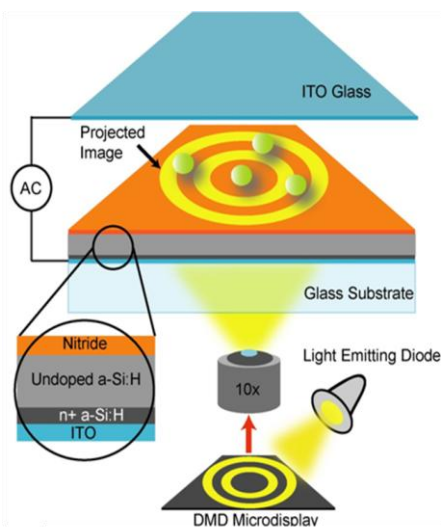


Fig. 1. OET use the selective illumination of a photoconductive layer to create 'virtual electrodes' for dielectrophoresis. Parallel manipulation of cells can be realized using projected optical images. [1]

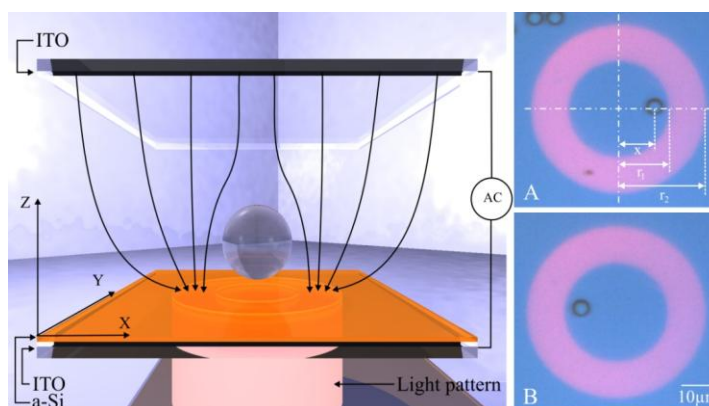


Fig. 2. An OET chamber consists of a liquid layer containing the beads sandwiched between two ITO-covered glass plates, one of which has a-Si covering it. When the stage is moved to the right (A) and then left (B), the particle is pushed in that direction. [15]



